


RealCycler®

Precision Microbiology

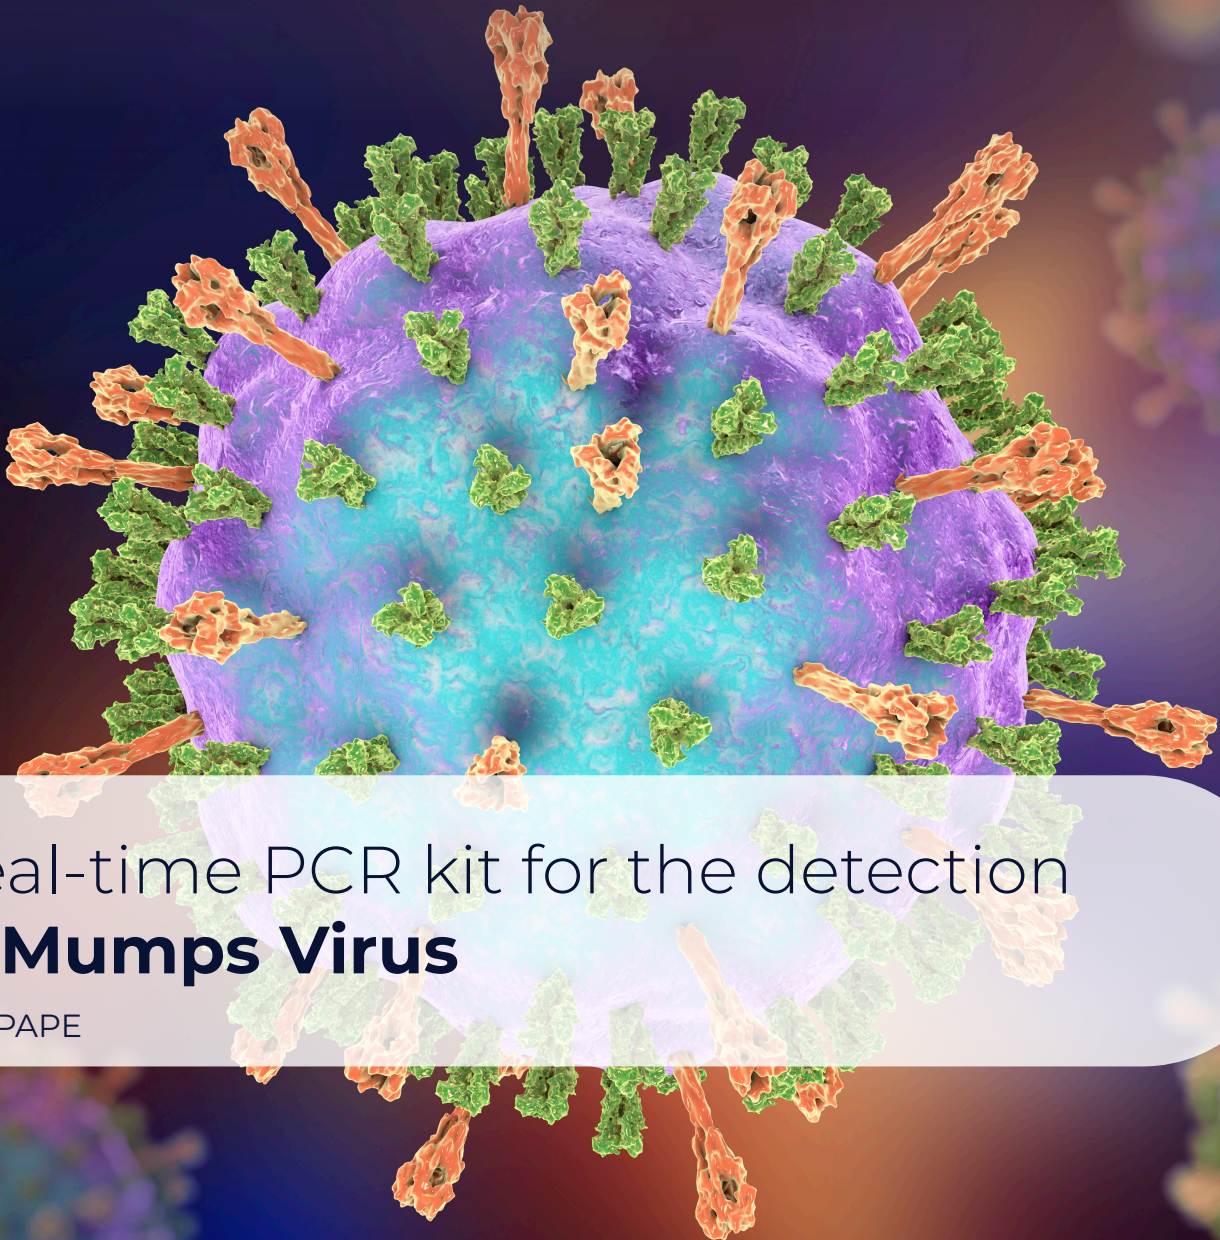

Real-time PCR kit for the detection
of **Mumps Virus**


Ref. PAPE

RealCycler[®] kits are based on Real-time PCR. No calculations or dilutions are required, just add the DNA/RNA of the sample and place it in the thermocycler.


RealCycler[®] PAPE allows the detection of Mumps Virus RNA in clinical samples. Mumps Virus infection causes parotitis, a disease characterized by swelling of the salivary glands. It can also involve other organs such as the pancreas, testes, ovaries, or central nervous system, leading to potential complications.

SPECIFICATIONS

- Ready to use: add the DNA/RNA and amplify.
- Internal Control (CHIC) is added to the sample to monitor DNA/RNA purification.
- Compatible with most DNA/RNA extraction systems.
- Clinical samples: cerebrospinal fluid, culture, nasopharyngeal exudate, saliva and urine and others.
- High sensitivity and specificity.
- Qualitative and quantitative.

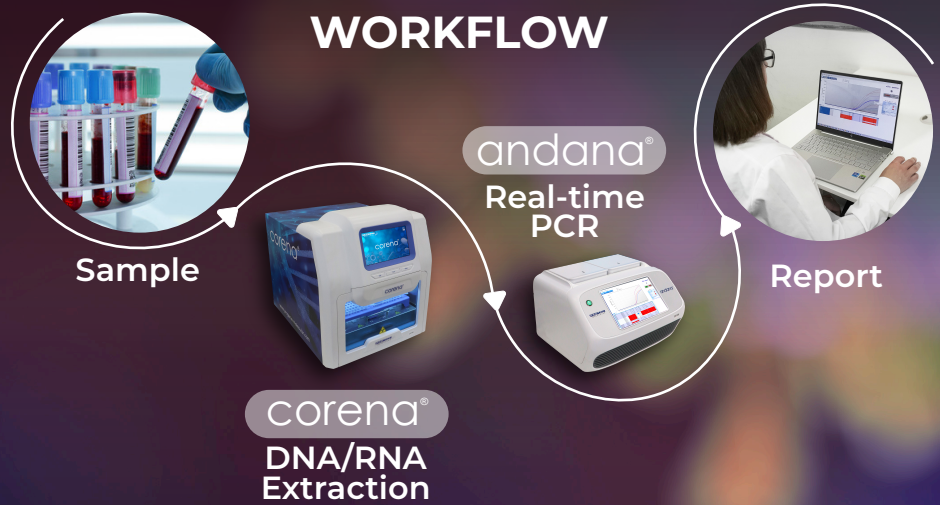

PRESENTATIONS

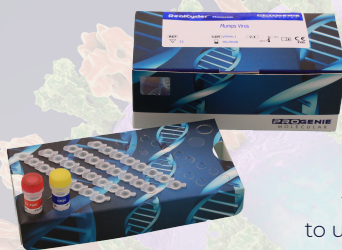


Monotest
Ref. PAPE-ABI32
The reagent is ready to use in 0.2 mL PCR tubes.



Universal
Ref. PAPE-UX
For the most common Real-time PCR instruments.

RESULTS INTERPRETATION

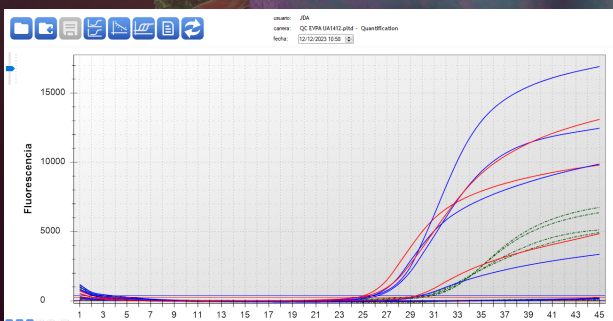

BioVisor Pro-Q software facilitates the interpretation of results obtained with *RealCycler* products for pathogens detection and quantification.

BioVisor Pro-Q imports fluorescence data from the Real-time PCR instrument, analyses them automatically and generates a report with the results.